


CONSTRUCTION TO BE DONE BY FACILITY:

- △ - 32" MINIMUM OPENING, 61" MINIMUM HALLWAY SWING CLEARANCE
- △ - MOUNTING SUPPORT BEHIND THE 3' X 3' 60LB TREADMILL CONTROL PANEL
- △ - 12" WIDE X 6" HIGH HOLE THROUGH WALL AS CLOSE TO FLOOR AS POSSIBLE
- ALL APPROVALS, PERMITS, AND AGENCY SUBMITTALS
- WET ENVIRONMENT WITH SPLASHING, DESIGN ROOM ACCORDINGLY
- AIR VENT 50CFM MINIMUM IN EACH ROOM WHERE EQUIPMENT IS LOCATED
- FLOOR BELOW TREADMILL FOOT PRINT TO BE LEVEL WITHIN .5" PER 7FT

PLUMBING TO BE DONE BY FACILITY:

- △ - 3" FLOOR DRAIN NEAR TREADMILL ENTRY RECOMMENDED
- △ - 12" X 12" RECESSED FLOOR DRAIN NEAR EQUIPMENT REQUIRED
- COLD WATER SUPPLY WITH HOSE BIB, FOR FILLING WATER STORAGE TANK
- HOT WATER WITH HOSE BIB FOR MAKEUP, TREADMILL & CARTRIDGE CLEANING

FACILITY LAYOUT:

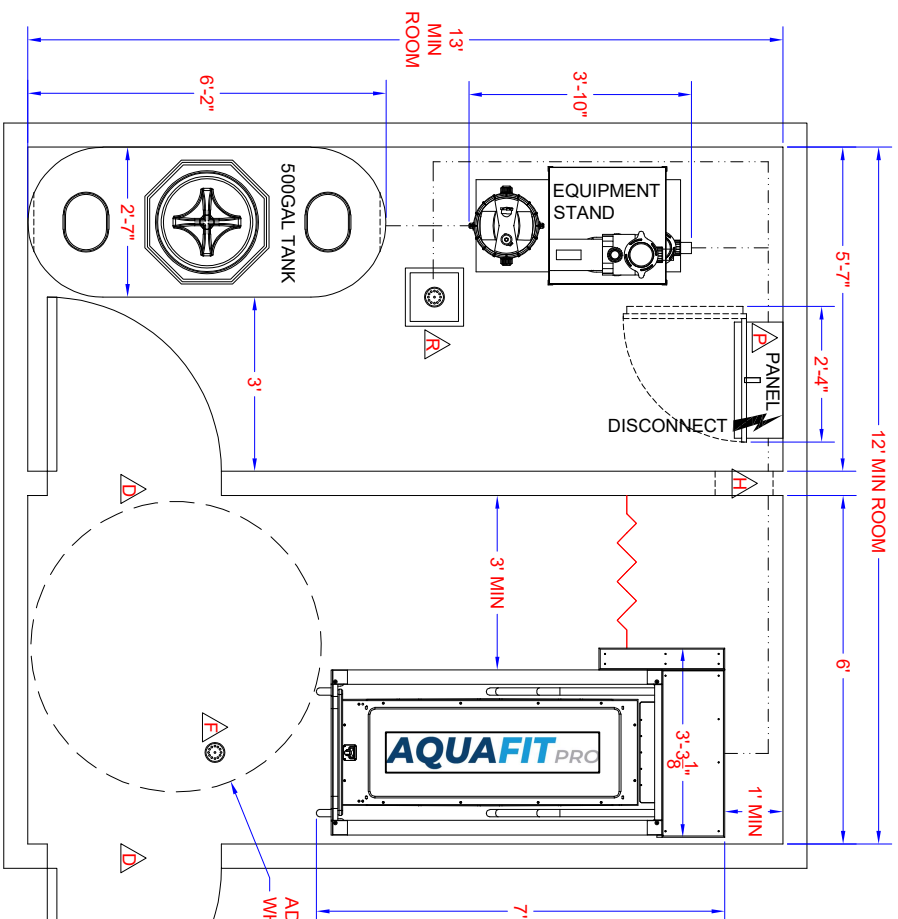

ELECTRICAL TO BE DONE BY FACILITY:

- 230V | 1PH | 60HZ | 50AMP | 4 WIRE ELECTRICAL SUPPLY WITH A SIEMENS GFI 50-AMP SPA PANEL, MODEL # W0408L1125SPA50 (REQUIRED)
 - SPA PANEL MUST BE WITHIN 10FT OR LESS OF TREADMILL CONTROL PANEL
 - EQUIPMENT WILL RUN BELOW 230VAC, BUT SHORTENS LIFE EXPECTANCY AND VOIDS WARRANTY (AN AQUABOOST TRANSFORMER P/N0789490 RAISES 20VAC)
 - MOUNT CONTROL PANEL AND CONNECT INCOMING POWER PER NEC CODE
 - AFTER INSTALL BOND ALL EQUIPMENT PER NEC CODE
- HUDSON SUPPLIED:**
- CUSTOM DESIGNED LAYOUT DRAWING WITH THE PURCHASE OF PRODUCT
 - INSTALLATION OF PURCHASED ITEMS AS PER FINAL SIGNED DRAWING
 - ON SITE IN-SERVICE TRAINING PROVIDED AFTER INSTALL
 - ELECTRICAL CONNECTIONS FROM PANEL TO HEATER, PUMPS, MOTOR, & HMI
 - "ASK SAM" WATER CARE SERVICE & AFTER HOURS SERVICE SUPPORT
 - PROPOSED PLUMBING PATH FROM TREADMILL TO EQUIPMENT
 - 3 FT DRIVE SHAFT CLEARANCE AREA FOR TREADMILL SERVICE

PURCHASED ITEMS:

0792001	AQUAFIT
500	GALLON TANK w/RECIRC.
0790200	2 SHELF EQUIPMENT STAND
0790802	EXTERIOR HAND RAILS AT ENTRY
OPTIONS - NOT INCLUDED:	
2182578	SIEMENS GFI 50-AMP SPA PANEL
0792002	RESISTANCE JETS
0790364-A	OZONE WATER SANITIZER
2810403	INSULATED 500 GAL TANK COVER
0790801	FOLD DOWN SEAT
0790007	WATER TANK AUTO FILL VALVE
2150004	LOSS OF POWER DRAIN VALVE
2810351	TREADMILL OUTDOOR COVER
1520909	100FT HMI CABLE UPGRADE

WEIGHTS:

TREADMILL EMPTY	1,250 LBS
TREADMILL w/48" WATER	5,400 LBS
500 GALLON TANK EMPTY	215 LBS
500 GALLON TANK w/WATER	4,500 LBS

FLOOR LOADS:

TREADMILL w/48" WATER	302 LBS PER SQ. FT.
500 GALLON TANK w/WATER	354 LBS PER SQ. FT.

--- EXAMPLE DRAWING SHOWN, CALL ENGINEERING FOR A CUSTOM LAYOUT ---

THIS DRAWING AND INFORMATION CONTAINED THEREON ARE CONFIDENTIAL AND THE PROPERTY OF HUDSON AQUATIC SYSTEMS, LLC. THEY ARE NOT TO BE REPRODUCED, DISTRIBUTED, DISCLOSED OR USED FOR ANY PURPOSE WITHOUT THE EXPRESS WRITTEN CONSENT OF HUDSON AQUATIC SYSTEMS.

DRAWN BY:	SALESMAN:	REV. DATE:	DRAWING #:	FACILITY NAME:
HJS	XXXXX XXXXX	4-2-24	XX-XXXX	AQUAFIT PRO SAMPLE (STANDARD) LAYOUT DRAWING

--- FINAL DRAWING SIGN OFF ---
 PRODUCT TO BE BUILT AND INSTALLED AS SHOWN:
 APPROVED BY: _____
 DATE: _____